



AFCEC-CX-TY-TP-2014-0010

MECHANICAL DETAILS FOR CONSTRUCTION OF A DRY AEROSOL DEPOSITION CASE

Robert Nichols

Universal Technology Corporation
1270 N. Fairfield Road,
Dayton, OH, 45432

FA4819-11-C-0003

July 2014

DISTRIBUTION A. Approved for public release; distribution unlimited. AFCEC-201434; 28 August 2014.

**AIR FORCE CIVIL ENGINEER CENTER
READINESS DIRECTORATE**

DISCLAIMER

Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not constitute or imply its endorsement, recommendation, or approval by the United States Air Force. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Air Force.

This report was prepared as an account of work sponsored by the United States Air Force. Neither the United States Air Force, nor any of its employees, makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights.

REPORT DOCUMENTATION PAGE					Form Approved OMB No. 0704-0188	
<p>The public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing the burden, to Department of Defense, Washington Headquarters Services, Directorate for Information Operations and Reports (0704-0188), 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to any penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.</p> <p>PLEASE DO NOT RETURN YOUR FORM TO THE ABOVE ADDRESS.</p>						
1. REPORT DATE (DD-MM-YYYY) 22-07-2014		2. REPORT TYPE Technical Paper		3. DATES COVERED (From - To) July 22nd 2014		
4. TITLE AND SUBTITLE Mechanical details for construction of a dry aerosol deposition device				5a. CONTRACT NUMBER FA4819-10-C-0003 X13SY002		
				5b. GRANT NUMBER		
				5c. PROGRAM ELEMENT NUMBER		
6. AUTHOR(S) Robert Nichols				5d. PROJECT NUMBER		
				5e. TASK NUMBER		
				5f. WORK UNIT NUMBER		
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Universal Technology Corporation, 1270 N. Fairfield Road, Dayton, OH 45432				8. PERFORMING ORGANIZATION REPORT NUMBER		
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) Air Force Civil Engineer Center Readiness Directorate Requirements and Acquisition Division 139 Barnes Drive, Suite 1 Tyndall Air Force Base, FL 32403-5323				10. SPONSOR/MONITOR'S ACRONYM(S) AFCEC/CXA		
				11. SPONSOR/MONITOR'S REPORT NUMBER(S) AFCEC-CX-TY-TP-2014-00xx		
12. DISTRIBUTION/AVAILABILITY STATEMENT Distribution A: Approved for public release; distribution unlimited.						
13. SUPPLEMENTARY NOTES Ref Public Affairs Case # 201434, 28 August 2014. Document contains color images.						
14. ABSTRACT This document contains detailed design information for assembly of a Dry Aerosol Deposition Device (DADD). This report is further to technical report AFRL-RX-TY-TP-2008-4617, ADA492108 and technical report AFRL-RX-TY-TR-2008-4592, ADA502105; work unit DODT0056.						
15. SUBJECT TERMS Dry Aerosol Deposition Device, Biological aerosols, spores, bacterial cells						
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT	18. NUMBER OF PAGES	19a. NAME OF RESPONSIBLE PERSON	
a. REPORT	b. ABSTRACT	c. THIS PAGE			Joe Wander; CXAE	
U	U	U	SAR	11	19b. TELEPHONE NUMBER (Include area code) 850 283-6240	

Reset

TABLE OF CONTENTS

LIST OF FIGURES	i
1. SUMMARY	1
2. INTRODUCTION	1
3. DESCRIPTION.....	1
4. REFERENCES	10

LIST OF FIGURES

Figure 1. Key components of a DADD	2
Figure 2. Mechanical drawing of replacement end cap; dimensions are given in inches.....	2
Figure 3. Mechanical drawing of replacement housing.....	3
Figure 4. Mechanical drawing for nozzle (DADD component 4)	3
Figure 5. Schematic of control unit connection.....	4
Figure 6. Mechanical drawing of dispensing system (DADD component 5).....	5
Figure 7. Mechanical drawing of dispensing system base.....	5
Figure 8. Mechanical drawing of Impinger top	6
Figure 9. Mechanical drawing of motor drive hub	6
Figure 10. Mechanical drawing of dispensing system turntable.....	7
Figure 11. Support stand (DADD component 6): comprising base (1), dryer support rear (2), dryer support front (3), and valve support arms (4).....	7
Figure 12. Mechanical drawing of support base (Support Stand Item1)	8
Figure 13. Mechanical drawing of dryer support rear (Support Stand Item 2).....	8
Figure 14. Mechanical drawing of dryer support front (Support Stand Item 3)	9
Figure 15. Mechanical drawing of valve support arm (Support Stand Item 4)	9
Figure 16. Mechanical drawing of support weldment (Support Stand Items 3 and 4)	10

1. SUMMARY

This document contains detailed design information for assembly of a Dry Aerosol Deposition Device (DADD). This report is further to technical paper AFRL-RX-TY-TP-2008-4617, ADA492108 and technical report AFRL-RX-TY-TR-2008-4592, ADA502105; work unit DODT0056.

2. INTRODUCTION

Growing threats of biological contamination of infrastructure and equipment led to the development of antimicrobial surfaces/coatings. Standard methods to test efficacy of such materials have applied microbial agents suspended in aqueous buffers. These surfaces, however, will likely be contaminated via aerosol exposure, so antimicrobial efficacy measurements using microbes deposited as aerosols will provide a more-representative test platform. A settling chamber is the most common method for depositing biological aerosols on surfaces, but it can impose limitations in respect to time and variability of sample loading. In prior work, a Dry Aerosol Deposition Device (DADD) was developed that uses impaction rather than settling to load surfaces with biological aerosols, providing a mechanism for rapid and highly reproducible loading of microorganisms onto surfaces. The DADD was tested with *Bacillus atrophaeus* spores and *Staphylococcus aureus* vegetative cells, deposited to glass coupons at concentrations exceeding 1×10^4 colony-forming units/cm². The average coefficient of variation (CV) for sample-to-sample loading within experiments was 13.6% for spores and 6.1% for *S. aureus* cells. The DADD provides a mechanism to load coupons with a highly reproducible challenge of microorganisms. Preliminary validation was performed on glass coupons, but the device can also be used with aluminum, concrete or fabric samples. The DADD was demonstrated to be a relatively simple and inexpensive device that can easily be contained within a 4-foot biological safety cabinet.¹

3. DESCRIPTION

Technical details for operation, validation, and analysis of biological aerosols using the DADD are provided elsewhere.¹ Preliminary construction of the DADD was reported previously, but detailed fabrication instructions and mechanical drawings are expanded herein. The DADD device consists of six key components (Figure 1): (1) a Collison nebulizer (BGI, Inc. Waltham, MA), (2) a diffusion dryer (Air Techniques International, Owens Mills, MD), (3) an M20-3GF02N5EG5 diverter valve (GC Valves, Integrated Process Solutions, Kennesaw, GA), (4) a nozzle and (5) a dispensing system. All components are assembled on a support stand (6) and connected to a control system (not shown). Dimensions in all drawings are US inch series (Imperial Units). Materials used for the construction of components referenced by the included mechanical drawings were aluminum alloy unless specified on the individual drawing.

The Collison nebulizer (1) was modified by welding a stainless steel 3/8-in \times 1/2-in National Pipe Thread (NPT) pipe bushing (SS-8-RB-6, Swagelok[®] Company) to the outlet pipe. This allowed use of a compression fitting (SS-810-7-8, Swagelok[®] Company) for connection to the diffusion dryer (Model 250, Air Techniques International (ATI)). The ATI diffusion dryer (Figure 2) uses plastic housing and end caps that are not suitable for steam sterilization. To achieve compatibility, new housing and end caps were fabricated from stainless steel and brass, respectively, to replace the original components (Figure 3 and Figure 4).

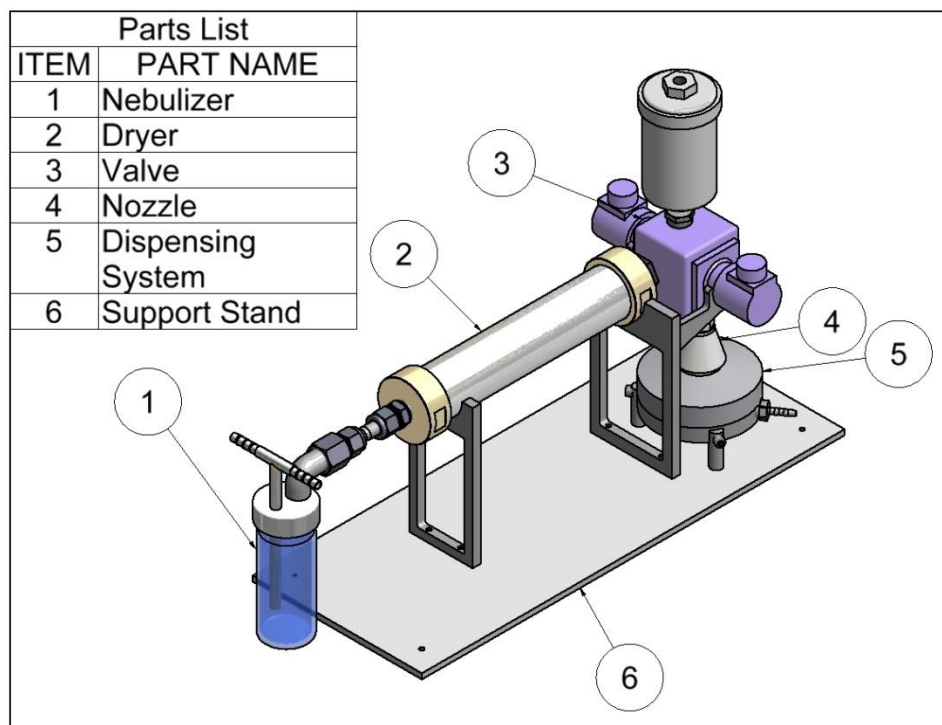


Figure 1. Key components of a DADD

NOTES:

1. 2 ea. req'd
2. Material may be Brass (ASTM B-21 Alloy 485 or equiv.) or Bronze (ASTM B-140 Alloy 316 or equiv.)

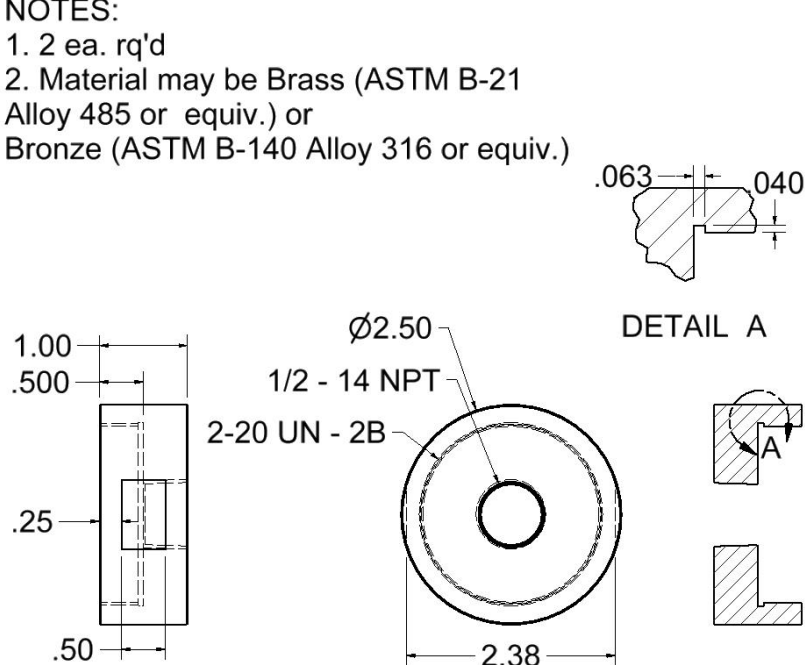


Figure 2. Mechanical drawing of replacement end cap; dimensions are given in inches

NOTES:
 1. 2" 304 Stainless
 Steel mechanical
 tubing
 2. Threads to fit
 caps free running

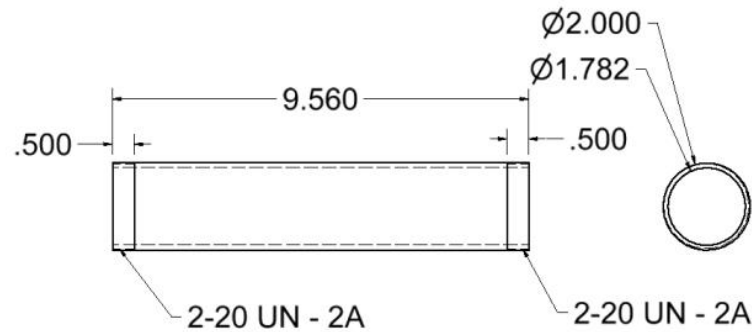


Figure 3. Mechanical drawing of replacement housing

Compression fittings (SS-810-1-8, Swagelok® Company) were used to connect the diffusion dryer to the nebulizer. A 1/2-in × 3/4-in NPT reducing pipe nipple (SS-12-HRN-8, Swagelok® Company) was used to connect the diffusion dryer to the inlet port of the diverter valve. The diverter valve was then attached to the diffusion dryer as described above.

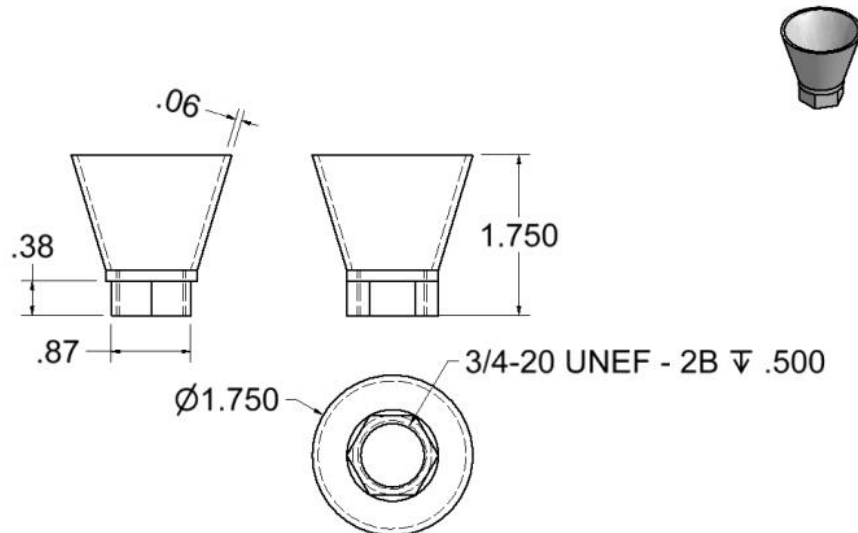


Figure 4. Mechanical drawing for nozzle (DADD component 4)

The normally open outlet of the diverter valve was positioned pointing upward and fitted with a HEPA filter (USA Numatics, Inc, Novi, MI) using a 1/2-in \times 3/4-in NPT reducing pipe nipple (SS-12-HRN-8, Swagelok[®] Company). The normally closed outlet was positioned pointing downward and fitted with a nozzle fabricated from aluminum stock(Figure 4) and using a modified male connector (SS-810-1-12, Swagelok[®] Company). The modification consisted of simply boring the male connector through to a 0.500-in diameter.

A control unit (Figure 5) was constructed to control the duration and interval of the diverter valve actuation and the rotation of the dispensing system.

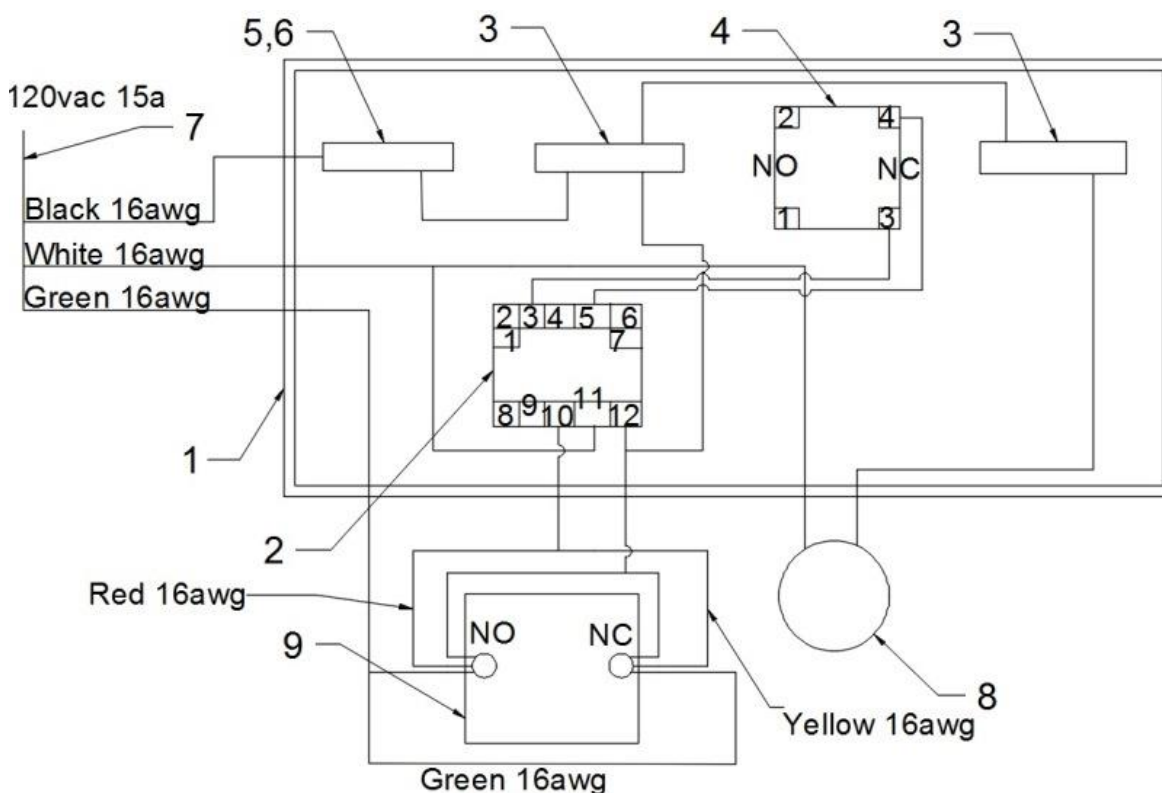


Figure 5. Schematic of control unit connection

Key: (1): Enclosure (Hubbell Wiegmann, Freeburg, IL, part # HW-100806CHSC), (2): Timer (Koyo Electronics, Tokyo, Japan, part # KT-V4S-D), (3): Switch (Hawkes Electronics, Wheeling, IL part #CA04J137207Q), (4) Switch (Baco Controls, Inc., Baldwinsville, NY part # unknown), (4.1) Contactor Kit (Baco Controls, Inc., Baldwinsville, NY part # unknown) (5): circuit breaker (Schurter Inc. Santa Rosa, CA part # 4430.2309), (6): circuit breaker cover (Schurter Inc. Santa Rosa, CA part # 4430.013), (7): power cord (Electri Cord Mfg Co. Eagan, MN part # PCLT66609), The following not shown in drawing, but used to connect components, (8): cord grip (Seacon LLC, Centennial, CO part #69915K54), (9): GC Valve (GC Valves, Integrated Process Solutions, Kennesaw, GA), (10): heat shrink tubing (Insultab Inc, Woburn, MA part # HS-105-3/8 in), (11, 12, 13): power connectors, black, white and green respectively (Anderson Power Products, Sterling, MA part # 1395G1S, 1395G2S, 1395G3S)

The dispensing system is composed of a control switch contained in a controller box, a 20-rpm gear motor (Polyvolt North Haven, CT; part # J206 XMC-6032), and components described in the mechanical drawings (Figure 6–Figure 10).

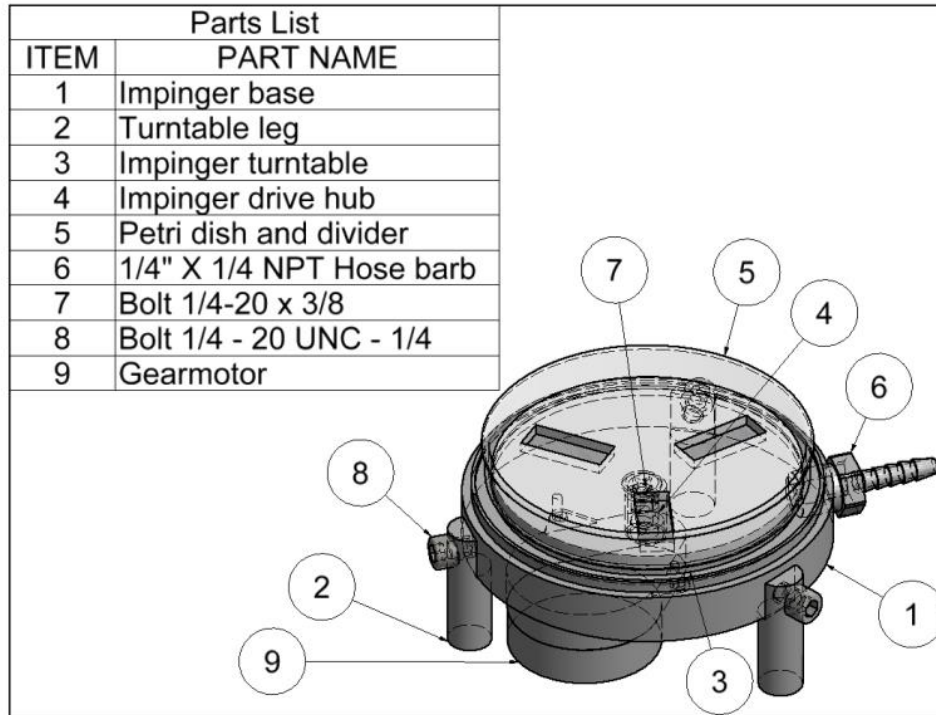


Figure 6. Mechanical drawing of dispensing system (DADD component 5)

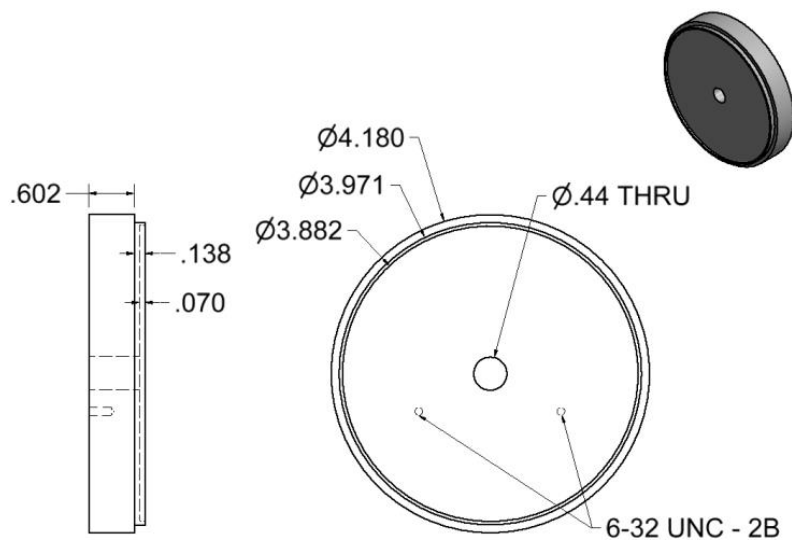


Figure 7. Mechanical drawing of dispensing system base

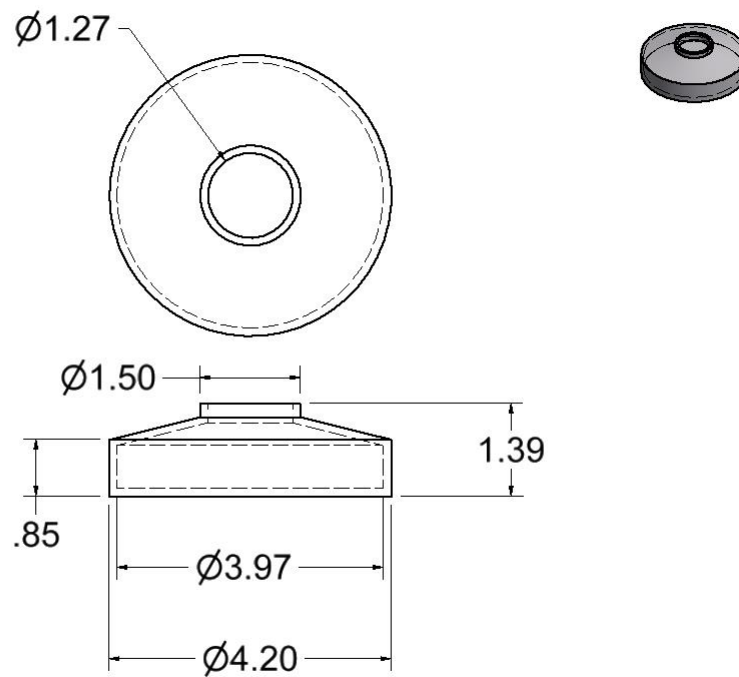


Figure 8. Mechanical drawing of Impinger top

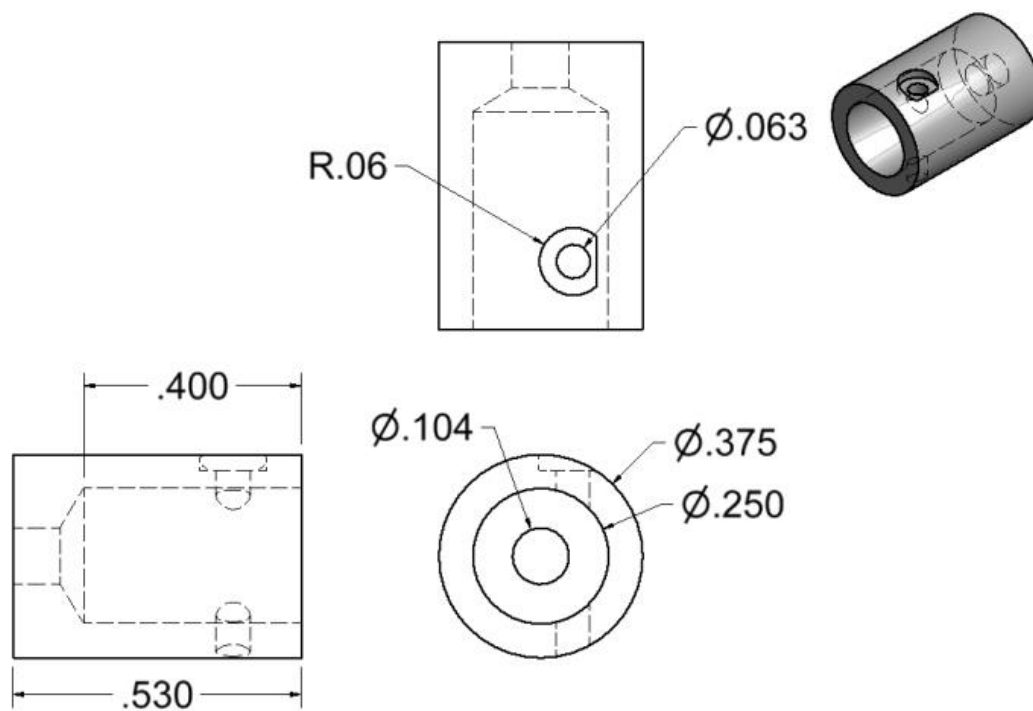


Figure 9. Mechanical drawing of motor drive hub

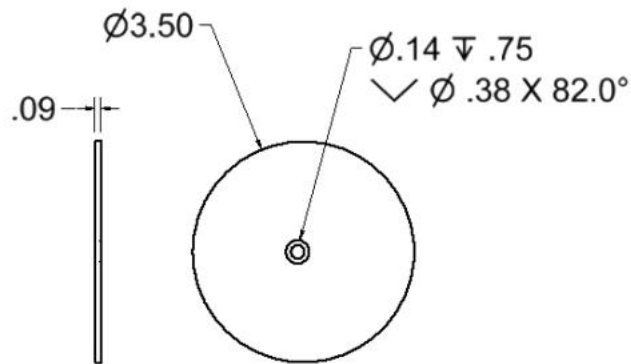


Figure 10. Mechanical drawing of dispensing system turntable

The support stand is composed of aluminum components described in the drawings (Figure 11–Figure 16).

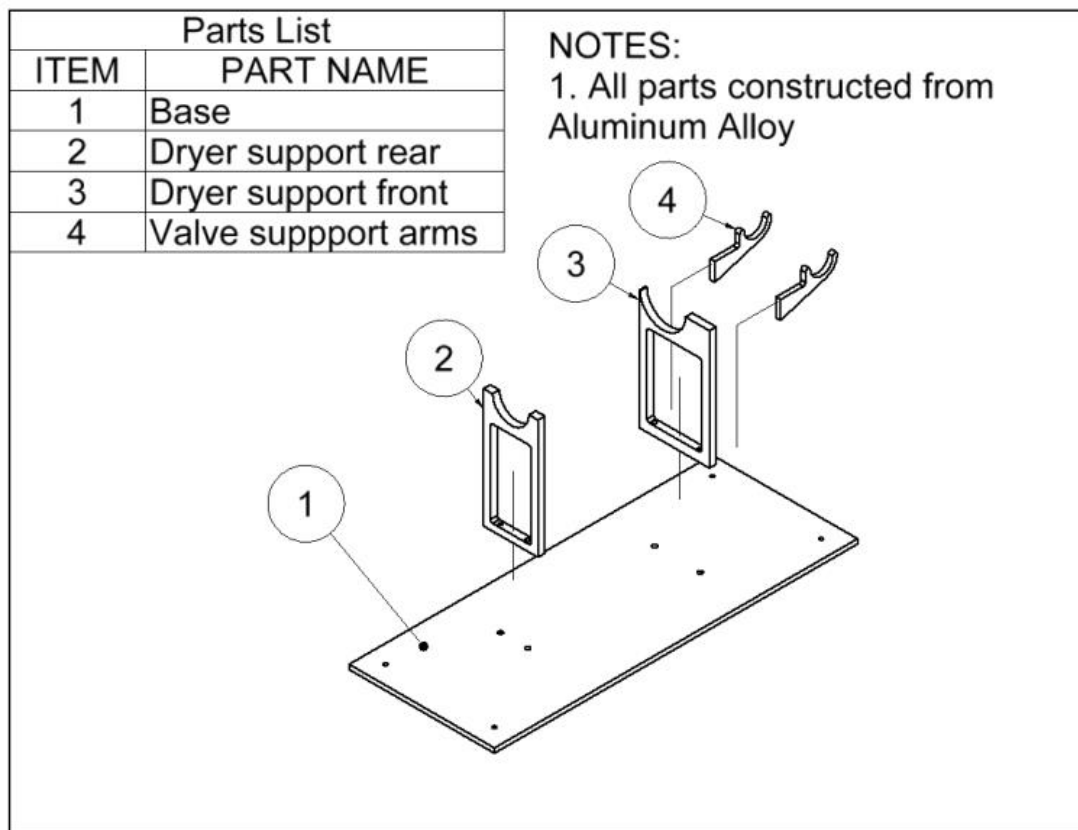


Figure 11. Support stand (DADD component 6): comprising base (1), dryer support rear (2), dryer support front (3), and valve support arms (4)

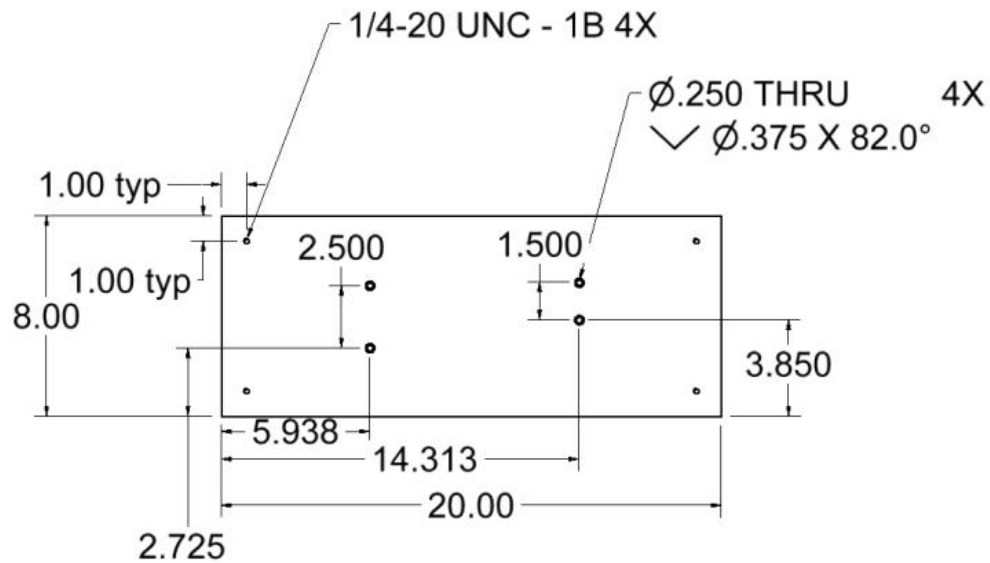


Figure 12. Mechanical drawing of support base (Support Stand Item1)

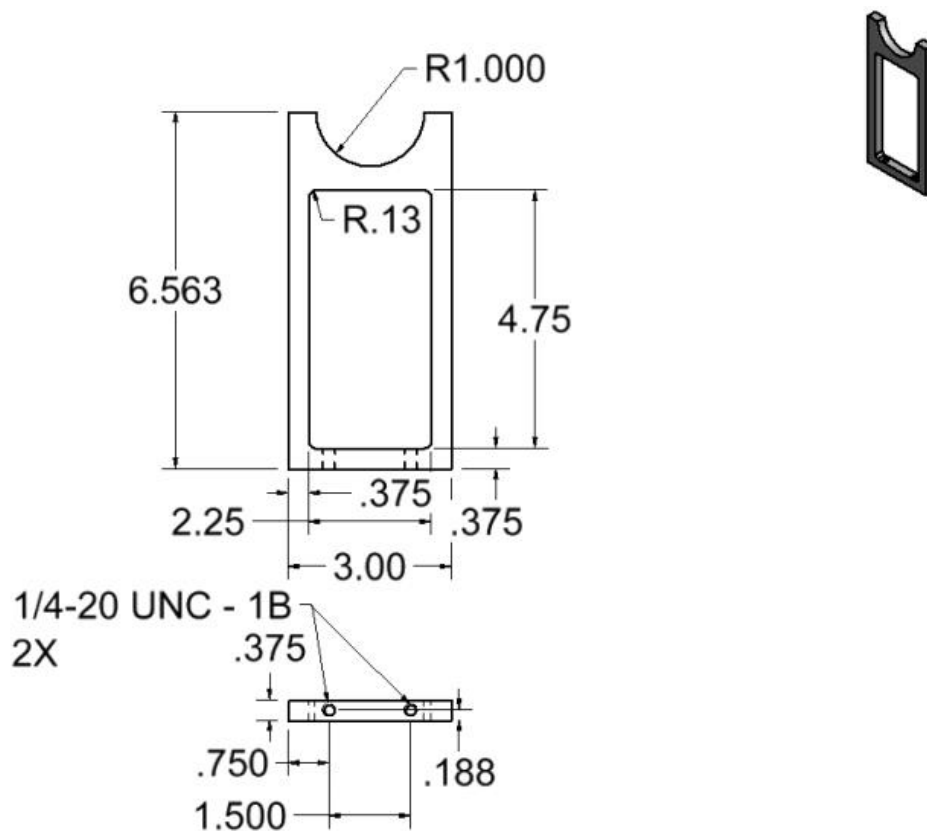


Figure 13. Mechanical drawing of dryer support rear (Support Stand Item 2)

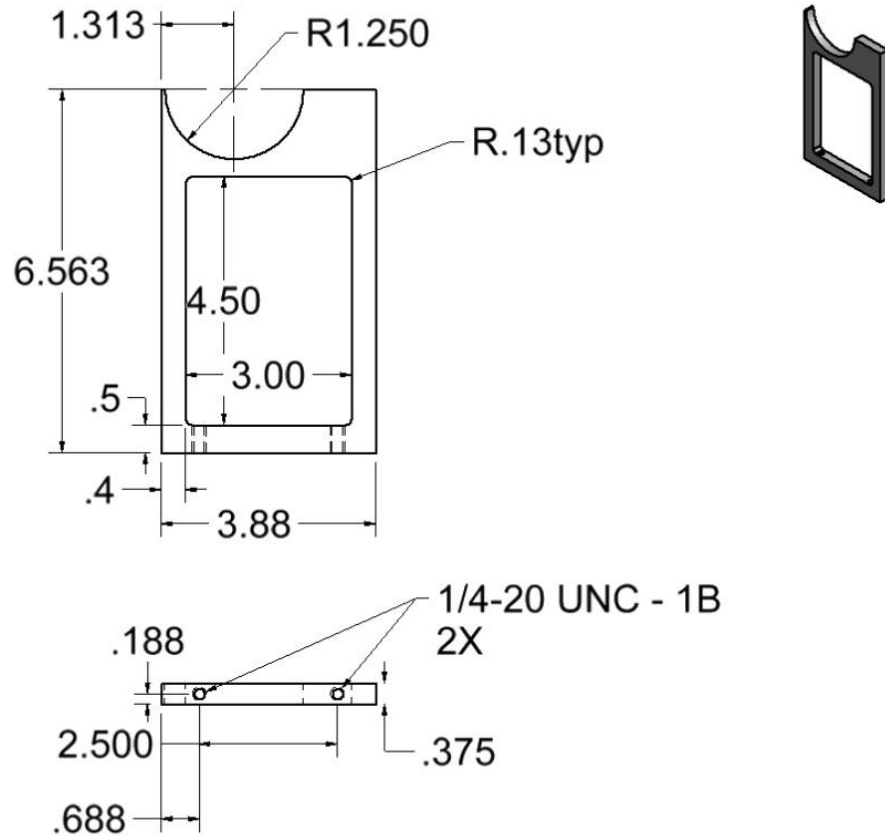


Figure 14. Mechanical drawing of dryer support front (Support Stand Item 3)

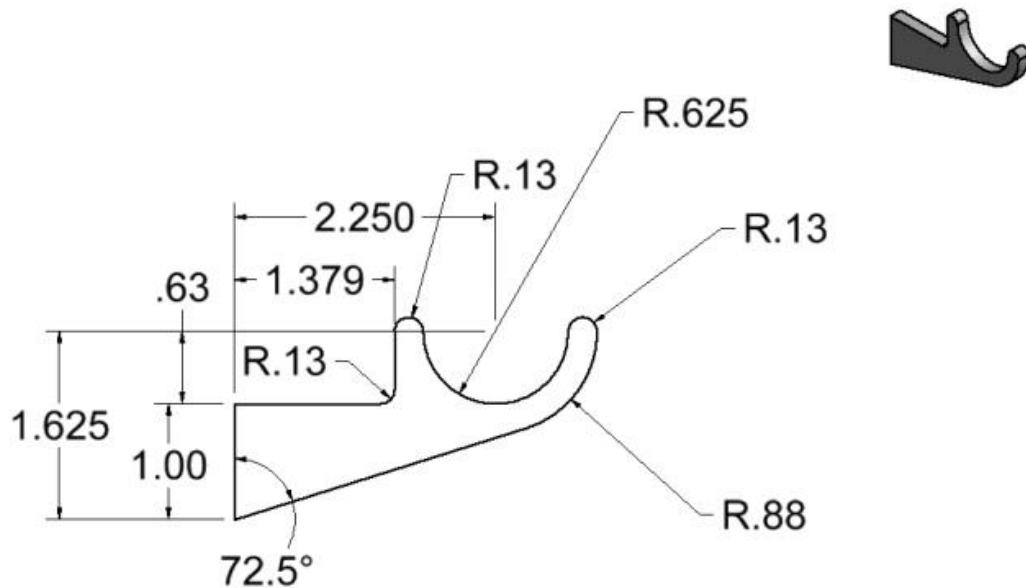


Figure 15. Mechanical drawing of valve support arm (Support Stand Item 4)

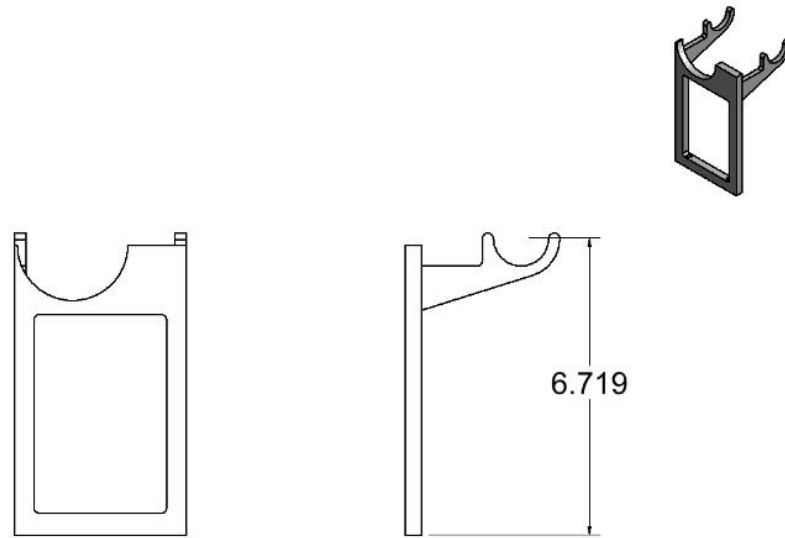


Figure 16. Mechanical drawing of support weldment (Support Stand Items 3 and 4)

4. REFERENCES

B.K. Heimbuch, K. Kinney, B. Nichols, J.D. Wander. The Dry Aerosol Deposition Device (DADD): An instrument for depositing microbial aerosols onto surfaces. *Journal of Microbiological Methods*, 78 (2009), 255–259